

# AP Forearm – Equipment Setup






# AP Forearm - Positioning

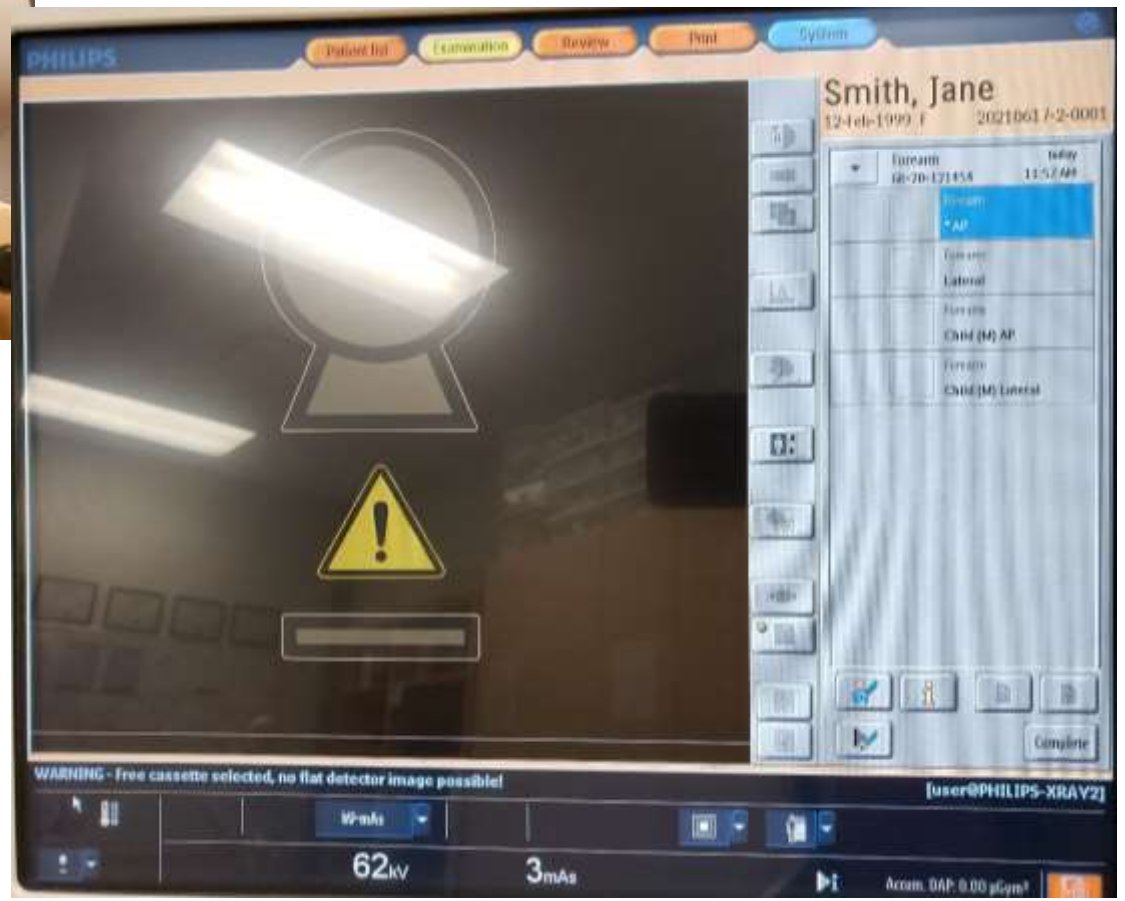


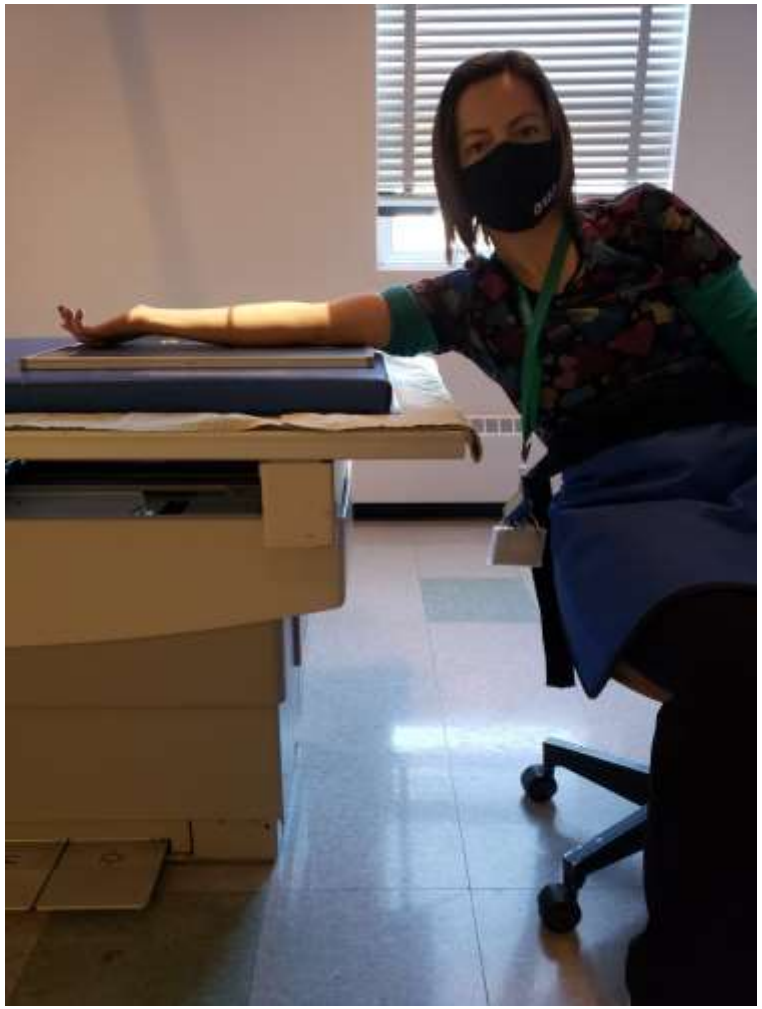
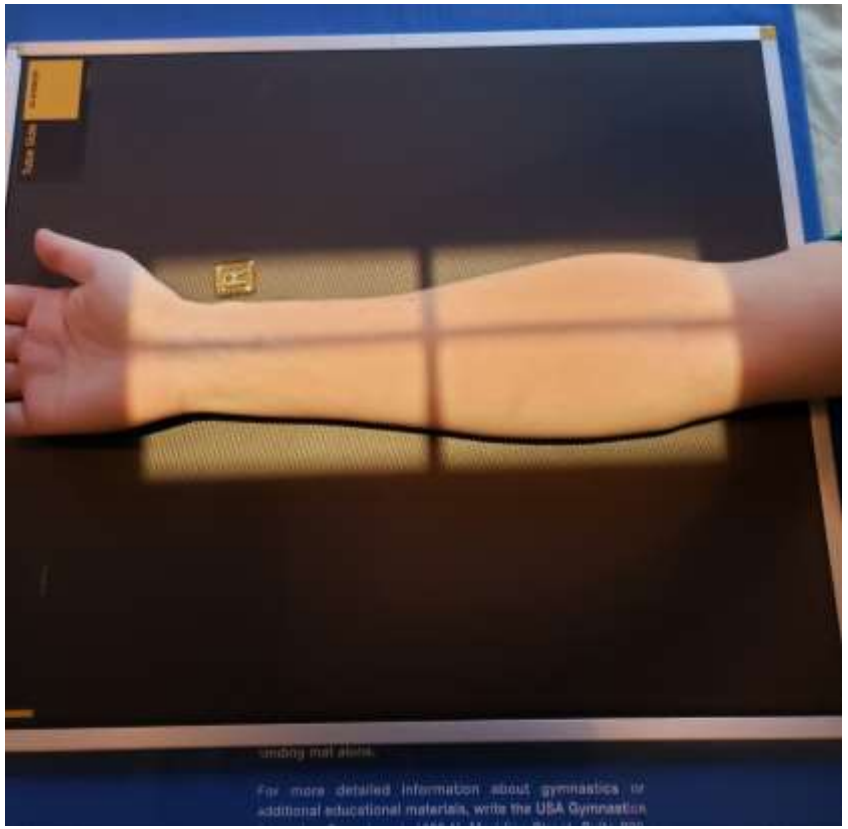
# Lateral Forearm – Equipment Setup



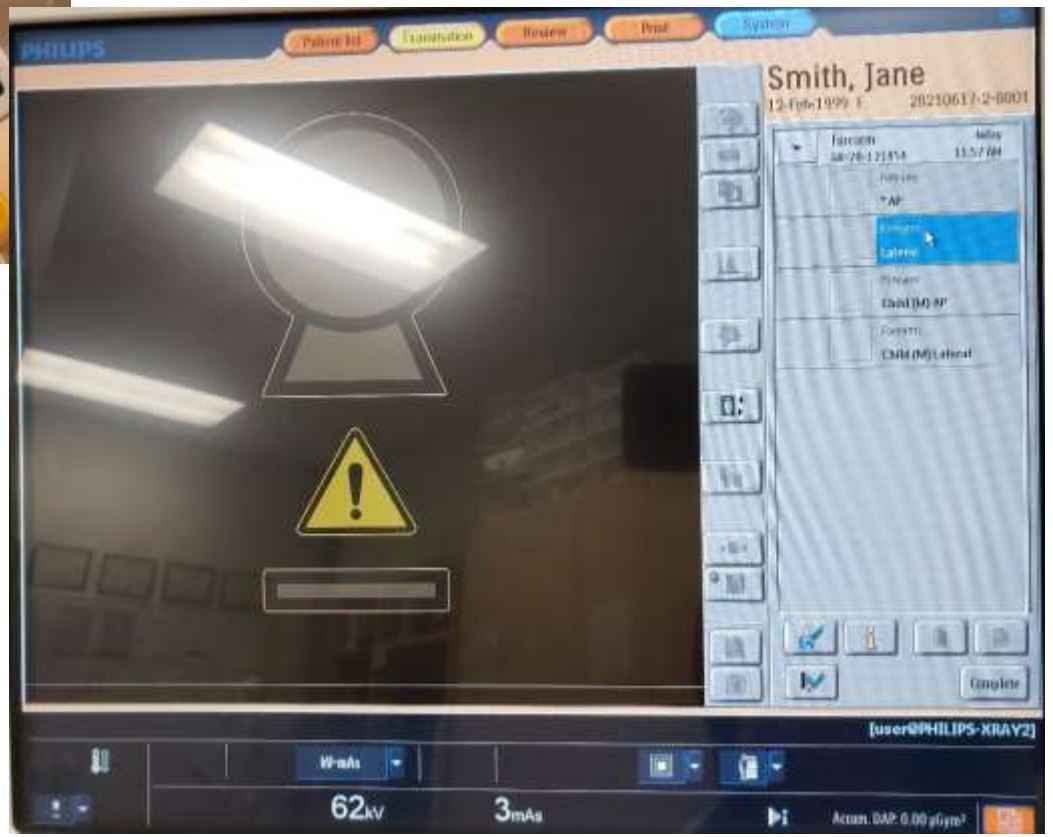

# Lateral Forearm - Positioning





# Notes

For all routine projections:

- 100cm SID is manually measured
- Bontrager recommended technique: 65-75kVp
- Lap shield placed over patients waist
- Large cassette was used
  - Cassette was changed after first exposure
  - Cassettes cleaned after dismissing the patient

# Copyright Information




- This learning material is property of edenbrook College.
- Any sharing, reproduction or use of this information or material other than educational purposes at edenbrook College is prohibited.